Wealden Rehab
Care Equipment Excellence

RAZ ART Shower Chair

Assessment Form



CELEBRATING 20 YEARS 2003-2023

APRIL 2023

1 Therapist and Users Details

Assessment Date:

Therapist Details

Name: .....

Organisation: .....

Email: .....

Telephone: .....

User Details

Name/Ref: .....

Address: .....

.....

.....

Email: .....

User Weight: .....

Notes: .....

.....

.....

Information

If you require assistance in completing this form, please call our sales office on 01634 813388, or use our online chat facility at www.wealdenrehab.com/chat

Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

2 Core Stock Chair

Core Stock Chair includes:

RAZ ART N6291 Frame

plus



N2581
Open Front Seat
18x16



N676
Standard Armrests



N720
Standard footplates



N731
Standard Headrest



N2581
Commode pan

Ordering details to include:

- **Seat Height**
- **Armrest Height**
- **Backrest Angle**
- **Seat adjustment (backrest movement)**

Information

Seat measurements can be configured on **pages 6 & 7**.

Set Up:

On delivery the prescriber is required to adjust:

- **Tension Adjustable Backrest**
- **Pelvic alignment**
- **Footplate Height**


Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

2 Chair Dimensions

Seat Width

1


Measure the outside of the users pelvis:

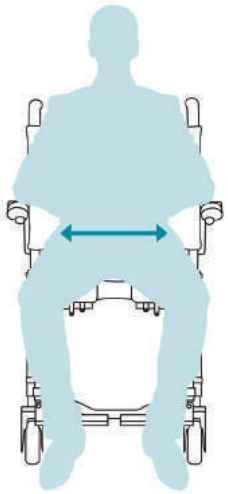

Fill in measurement:

2

ART Standard range
450mm

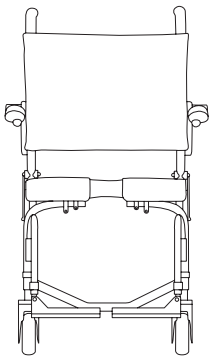

160kg ART Standard Range


accommodates a hip width of 400mm - 520mm

☑ **CORE STOCK ITEM**

Arm Height

3

Specify arm height (default position is 248mm)

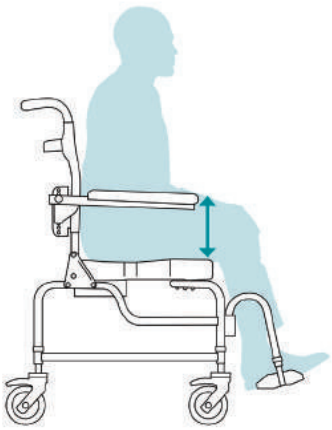


L		R
☐	200mm	☐
☐	212mm	☐
☐	224mm	☐
☐	236mm	☐
☐	**248mm**	☐
☐	260mm	☐
☐	272mm	☐

Backrest Angle

4

Specify backrest angle (default position 90°)

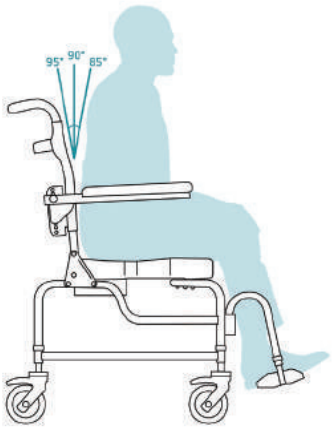

☐ **90°**

☐ 95°


Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

2 Chair Dimensions

Seat Depth

5

Measure user's back to back of knee:

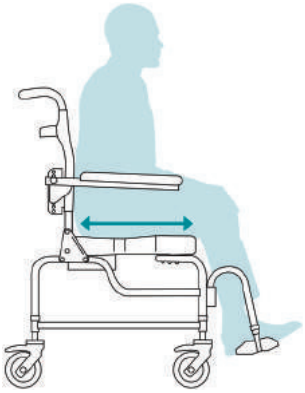

Fill in measurement:





(Ideal chair depth)

Information

Need extra pressure relief? See **page 9** for additional seat options.

6

Select which seat will best suit the user:

	Length / Aperture Design	Bridged Seat Bridged front design removes the risk of the users' leg falling into the gap of the seat – so consider this one for thinner users. Ideal for users with involuntary movement or those performing a side transfer.	Open Front Seat The open front seat gives the user and carer more access for personal hygiene. Opt for this seat when access is required and there is no risk of legs becoming entrapped in the gap.
185kg AT Standard	**400m** Adjusts to accommodate 380 – 440mm seat depth	☐ N0007 	☑ **CORE STOCK ITEM** N0006 
	475mm Adjusts to accommodate 450 – 500mm seat depth	☐ N0009 	☐ N0008 


Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

2 Chair Dimensions

Seat Height

7

When choosing the seat height consider clearance required for the toilet, side transfer or standing transfer heights.

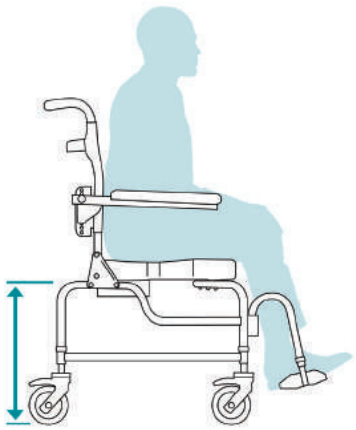

Toilet Bowl Height: (seat up)

.....

Chair Seat Height:


.....

Toilet bowl height (mm)	**360**	**380**	**400**	**420**	**440**	**460**	**480**	**500**	**520**	**540**	**560**
ART Standard Seat Height	500	530	530	560	560	580	610	640	640	660	685

Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

2 Chair Dimensions

Lining up your chair with the toilet bowl

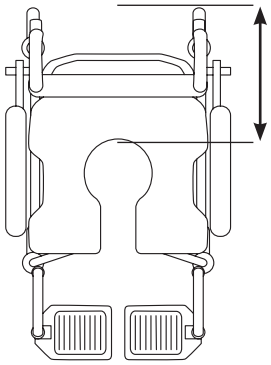

Rearmost chair point to rear of seat aperture

AP = 180mm

ART = 230mm

SP = 280mm

AT = 340mm

Using an automatic WC?

Geberit:

All RAZ chairs are compatible with the Geberit Mera Care toilet.

For the Geberit 7000 and Aquaclean 8000, the RAZ ATW, RAZ ART and AP Auto provide the best fit.

Closomat:

For a tilt in space chair, the RAZ ATW and RAZ-ART fit well over the Closomat toilet.

For an attendant and self-propel option, we suggest using the RAZ-AP Auto, this can also be upgraded with a self-propel wheel kit.

Bio-Bidet:

RAZ chairs are not compatible with the BioBidet.


Best practice

A common requirement is to have the skirt accessory added to the underside of the seat and the option of removing the pan sliders to provide a closer fit with the toilet. The standard moulded seat shaping contributes to a much improved wash experience.

Footplate Height

8

Measure user's lower leg length:

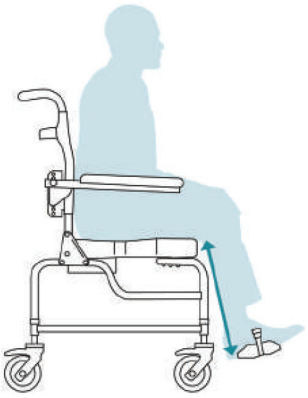

Seat to Footplate Dimension:

(Standard 400-520mm)

Information

If the standard footplates are not suitable - see the accessories list of footplates on **page 8**.



RAZ skirt accessory

Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

3 Accessories – Additional Cost

Footplate Accessories*

☑ 

N720 – Standard Footplates, pair, Adjustable 41-52cm, with folding plate.

CORE STOCK ITEM

☐ 

N2628 – Neoprene Footplate Covers, for RAZ Standard Footplates. To give a softer texture under the users foot.

☐ 

N722 – MFX Footrests for RAZ Rehab Shower Chair, pair, minimal forward extension, adjustable 300-410mm. For users with a lower leg length between 300-410mm.



50mm offset footrest receivers

☐ **N7301L** – Left

☐ **N7301R** – Right

☑ 

N2632 – Calf strap to give the legs support when the chair is tilted and to prevent feet from slipping backwards.

☐ 

N721 – MFX Footrests for RAZ Rehab Shower Chair, pair, minimal forward extension, adjustable 200-300mm. For users with a lower leg length between 200-300mm.

☐ 

N724 – Angle Adjustable Footplates for RAZ Rehab Shower Chair. Footplate can be angled to accommodate users with footdrop or if the ankle is in a fixed position.

☐ 

N2632 – Bodypoint Aeromesh Calf Strap.



☐ **N715** – Elevating Legrest for RAZ Rehab Shower Chair to suit 450mm seat depth – Left side

☐ **N718** – Right side



☐ **N716** – Elevating Legrest for RAZ Rehab Shower Chair to suit 575mm seat depth – Left side

☐ **N719** – Right side

N715/718/716/719 – The footplate elevates to support a leg that may be in extension. It also offers calf support. The options are for left and right and also for either a 400mm seat depth cushion or a 475mm seat depth.


*Additional charge

Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

3 Accessories – Additional Cost


Pressure Relief Seats*

Visco Seat Options:

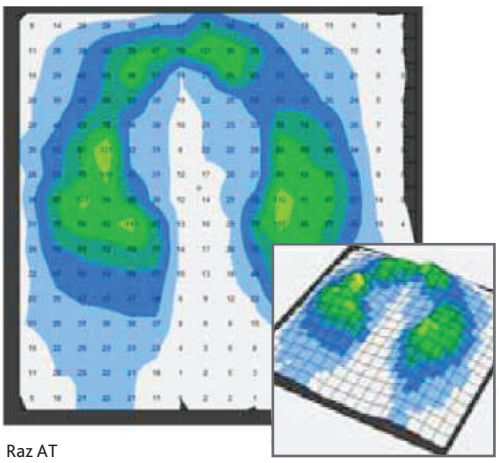


Raz AT

The Visco Seat option offers additional pressure relief for the user, and is recommended for those who suffer from pressure sores or are at high risk of acquiring one. These seats also give the option of side or rear access, which cannot be achieved with the standard range of seats.



Aquatec



Freeway T80

136kg AT Standard Range	Length / Aperture Design	Bridged Seat	Open Front Seat	Open Left Seat	Open Right Seat	Open Rear Seat
	400mm Adjusts to accommodate 380 – 440mm seat depth	N650	N651	N652	N653	N654
	475mm Adjusts to accommodate 450 – 500mm seat depth	N655	N656	N657	N658	N659

☐ No Pressure Relief Seat

Information

If you are ordering the AT600 Shower chair, please call us on **01634 813388** for advice on Visco seats.

*Additional charge

Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

3 Accessories – Additional Cost

Postural Support Accessories*

☐ 

N690 – Swing-away Lateral Supports for RAZ Shower Chair, pair, complete with adjustable lateral pad and neoprene support wrap. These give thoracic support to the patient's torso, helping to keep their posture upright. They can be adjusted in height/depth and angle.

☐ 

N703 – Hip adductors

Headrest Support Accessories*

☑ 

N731 – Standard headrest.

CORE STOCK ITEM

☐ 

C5960 – Head support cushion. This head cushion is flexible so can be curved around the users head. Comes with a stem to give height and depth adjustment.

☐ 

C5961 – Head support cushion. Very solid head support for clients who cannot support their own head. This support is not flexible.

☐ 

C5963 – Head support cushion. Most common headrest for users needing lateral support for their head. This is flexible so can wrap around the sides of the head to help support it in an upright position.

☐ 

N3906 – RAZ Headrest Clamp with 75mm Side-To-Side Offset Adjustment – specify this if the support required is not in the centreline of the chair.

☐ 

N3761 – Type G headrest
The Type G headrest provides maximum comfort and support to the back and sides of the head or neck area. It can be adjusted to meet the changing needs of the wheelchair occupant.

*Additional charge

Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

3 Accessories – Additional Cost

Chair Accessories*

Arms

☑ 

N676 – Standard Armrests
Flip-up for easy access and transfers (come as part of Adjustaback)

CORE STOCK ITEM

☐ 

N676 – Armrest Lock Kit for RAZ Rehab Shower Chair, pair. This kit stops the armrest moving up and therefore can be used for the patient to pull on and re-position. The lock releases to allow the arm to lift freely.

☐ 

N681 – These arm troughs help to keep the arm on the pad without falling off. There is angle and depth adjustment to the pads to suits the position of the users arms.

☐ 

N679 – Wide Soft Armpad for RAZ Rehab Shower Chair, 350mm x 80mm – Pair. This armrest offer a wider area of support for the patient's arms.

☐ 

N683 – Pivoting Arm Mount – Pair. These are used in conjunction with product codes N681 and N679, in order to allow the armpad to rotate through 90° and move into the upright position without conflicting with the backrest.

Commode Pan

☑ 

N2581 – Commode Pan with handle and lid. Autoclavable.

CORE STOCK ITEM

Chest Harness

☐ 

Flex-Contol harnesses offer a greater range of posture
5.71032 – Mens
5.71034 – Womens

Pommel

☐ 

N3877 – RAZ Boris Pommel incorporating urine deflector.

☐ 

N6056 – RAZ adjustable Pommel. A safe and secure way of keeping the legs abducted, encouraging better posture control.

Lap Belts

☐ 

6.70002 – Squeeze-release bucking with single adjustment

*Additional charge


Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab

4 Sizing Guide


Dimension Chart – ART




Max Patient Weight
160kg

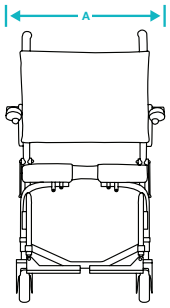


A Overall Width
570mm

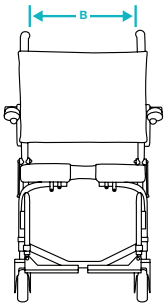


B Width between handles
400mm




C Height from top of seat to top of backrest vinyl
500mm




D Height from floor to top of push handles*
1100mm




E Top of seat from floor
560 / 580 / 610 / 640mm




F Underside of chassis side cross bar
180mm




G Height of arm above seat
200 – 260mm




H Depth of chassis
450mm




I Overall depth without footrests
620mm




J Overall depth with footrests
870mm




K Top of seat from standard footplates
410 – 520mm




L Rearmost chair point to rear of seat aperture
230mm



M Front of chassis to front of footplates
250mm



N Overall depth with footplates, in full tilt
1300mm



O Maximum clearance for WC cistern*
930mm

Care Equipment Excellence
01634 813388
hello@wealdenrehab.com
www.wealdenrehab.com
wealdenrehab